

One Step MET-THC Urine Rapid Test Kit

Instructions For Use

PRODUCT NAME

One Step MET-THC Urine Rapid Test Kit

PACKAGE SPECIFICATION

25 tests/kit

INTENDED USE

FRENOVO One Step MET-THC Urine Rapid Test is a lateral flow, qualitative immunoassay. It is intended for qualitative detection of Methamphetamine and Marijuana metabolite in human urine samples at the following cut-off concentrations:

Test Name	Calibrator	Cut-off
Methamphetamine(MET)	D-Methamphetamine	1000ng/ml
Marijuana (THC)	11-nor- Δ^9 -THC-9 COOH	50ng/ml

SUMMARY AND PRINCIPLES OF THE PROCEDURE

FRENOVO One Step MET-THC Urine Rapid Test uses the highly specific antibody & antigen reaction principle, as well as immunochromatography and colloidal gold labeling technology.

The test kit contains drug metabolites antibodies labeled with colloidal gold, and drug metabolites antigens which is fixed in the test area (T/M) on the membrane. When the urine sample was dropped into the sample well, the urine sample was then chromatography upward under capillary effect. If the concentration of drug metabolite in urine is lower than the cut-off level, the colloidal gold antibody can not be combined with all drug metabolites. In this way, the colloidal gold antibody binding will be bound by drug metabolite antigen fixed on the membrane during the chromatography, and a purple red band will appear in the test area (T/M). If the concentration of drug metabolite in urine is higher than the cut-off level, the colloidal gold antibody is bound to drug metabolite, so that in the test area (T/M) there is no purple red band because the competitive reaction does not bind to drug metabolite antigen. Whether drug metabolite is present in urine, a purple red strip will appear in the quality control area (C). The purple red band in the quality control area (C) is the standard to determine whether there is enough urine sample, whether the chromatography process is normal, and also as the internal control standard of tests.

MATERIALS PROVIDED

Each kit contains:

1. Test Devices: 25 pieces test devices individually pouched.
2. Droppers: 25 pieces droppers of 25 ul
3. Package insert: 1 piece attached.

MATERIALS REQUIRED BUT NOT PROVIDED

- Timer or stopwatch.
- Specimen collection containers
- Disposable gloves and/or protective clothing
- Micropipette

WARNINGS

1. Read the package insert completely before using the product. The instructions must be followed carefully as not doing so may result in inaccurate results.
2. FRENOVO One Step MET-THC Urine Rapid Testis for diagnostic use only.
3. Perform test at room temperature.

PRECAUTIONS

1. FRENOVO One Step MET-THC Urine Rapid Test is for professional use only.
2. The package insert instructions must be followed to ensure optimum test performance.
3. The used test device should be discarded according to local regulations.

Handling Precautions

1. Do not use if the kit box safety seal is absent, damaged or broken.
2. Do not use any device if the pouches have been perforated.
3. Each device is for single use only.
4. Do not use the kit past the expiration date (this date is printed on the kit box).
5. Adequate lighting is required to read the test results.
6. The result should be read immediately after the end of the 5 minutes incubation time following the addition of specimen and wash buffer solution. Do not read results beyond 10 minutes.

STORAGE INSTRUCTIONS

1. FRENOVO One Step MET-THC Urine Rapid Testkit should be stored between 2-30°C and the shelf life is 24 months.
2. If stored refrigerated, ensure that the pouched device is brought to room temperature before opening.
3. Do not freeze the kit.

SAMPLE COLLECTION AND PREPARATION

The urine specimen must be collected in a clean and dry container. Urine collected at any time of the day may be used. Urine specimens exhibiting visible precipitates should be centrifuged, filtered, or allowed to settle to obtain a clear supernatant for testing. Urine specimens may be stored at 2-8 ° C for up to 48 hours prior to testing.


QUALITY CONTROL

An internal procedural control is included in the test. a colored line appearing in the control line region (C) is an internal valid procedural control, it confirming adequate membrane wicking. Control standards are not supplied with this kit; however, it is recommended that positive and negative controls be tested as a good laboratory practice to confirm the test procedure and to verify proper test performance.

TEST PROCEDURE

Allow the test, urine specimen, and/or controls to reach room temperature (15-30°C) prior to testing.

1. Bring the pouch to room temperature before opening it. Remove the test device from the sealed pouch and use it as soon as possible.
2. Place the test device on a clean and level surface. Hold the dropper vertically and transfer 2~3 full drops of urine (approx. 50 ~75µL) to the specimen well of the test device, and then start the timer. Avoid trapping air bubbles in the specimen well. See the illustration below.
3. Wait for the colored line(s) to appear. Read results at 5 minutes. Do not interpret the result after 10 minutes.

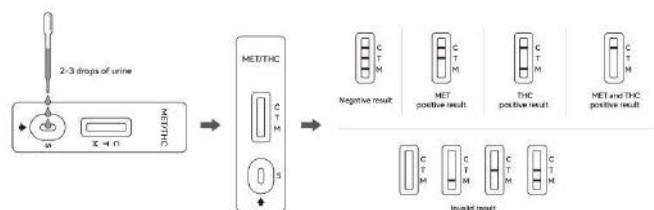

INTERPRETATION OF RESULTS

(Please refer to the illustration above)

NEGATIVE:* : The presence of three colored lines (M, T and C) within the result window, regardless of the order in which the lines appear, indicates a negative result. A negative result indicates that the drug metabolite concentrations are below the detectable levels.

***NOTE:** The shade of color in the test line region (T/M) will vary, but it should always be considered as negative whenever there is even a faint colored line.

Methamphetamine positive : The presence of both the THC test line (T) and the control line (C) within the result window, regardless of which line appears first, indicates a methamphetamine-positive result. This result indicates that the concentration of methamphetamine in the sample is at or above the detectable level (1,000 ng/ml).

THC positive : The presence of both the MET test line (M) and the control line (C) within the result window, regardless of which line appears first, indicates a THC-positive result. This result indicates that the concentration of THC metabolites in the sample is at or above the detectable level (50 ng/ml).

Methamphetamine and THC positive : The presence of only the control line (C) within the result window indicates a positive result for both methamphetamine and THC. This result indicates that the concentrations of methamphetamine and THC metabolites are at or above their detectable levels (1,000ng/ml and 50 ng/ml, respectively).

INVALID: Control line (C) fails to appear. Insufficient specimen volume or incorrect procedural techniques are the most likely reasons for control line failure. Review the procedure and repeat the test using a new cassette. If the problem persists, discontinue using the lot immediately and contact your local distributor.

LIMITATIONS

1. FrenoVO One Step MET-THC Urine Rapid Test provides only a qualitative, preliminary analytical result. A secondary analytical method must be used to obtain a confirmed result. Gas chromatography/mass spectrometry (GC/MS) is the preferred confirmatory method.
2. There is a possibility that technical or procedural errors, as well as other interfering substances in the urine specimen may cause erroneous results.
3. Adulterants, such as bleach and/or alum, in urine specimens may produce erroneous results regardless of the analytical method used. If adulteration is suspected, the test should be repeated with another urine specimen.
4. A positive result does not indicate level or intoxication, administration route or concentration in urine.
5. A negative result may not necessarily indicate drug-free urine. Negative results can be obtained when drug is present but below the cut-off level of the test.
6. The test does not distinguish between drugs of abuse and certain medications.
7. A positive result may be obtained from certain foods or food supplements.

PERFORMANCE CHARACTERISTICS

Positive cutoff reference range

According to the requirements of American drug abuse and mental health service administration (SAMHSA) for the cut-off value of Methamphetamine in

urine, the detection threshold of MET is set at 1000ng / ml and the cut-off value of Marijuana in urine, the detection threshold of THC is set at 50ng / ml.

Sensitivity and Specificity

Accuracy

A clinical study was conducted using FrenoVO One Step MET-THC Urine Rapid Test and GC/MS. Testing was performed on 150 pieces positive urine specimens and 150 pieces negative urine specimens previously collected and confirmed by GC/MS. The results indicated that FrenoVO One Step MET-THC Urine Rapid Test has a high sensitivity and specificity as summarized below:

clinical study		GC/MS		
FrenoVO One Step MET-THC Urine Rapid Test	Results	Positive	Negative	Total Results
	Positive	150	0	150
	Negative	0	150	150
Total Results		150	150	300

Accuracy Results:

Clinical sensitivity > 99.00 % (95%CI* 98.02 % to 100.0 %)

Clinical specificity > 99.00 % (95%CI* 98.02 % to 100.0 %)

Accuracy > 99.00 % (95%CI* 99.00 % to 100.0 %)

Analytical Sensitivity

A piece of drug-free urine was spiked with drugs to the concentrations at $\pm 50\%$ cut-off and $\pm 25\%$ cut-off. Each titer was repeated 30 pieces of test. The results are summarized below.

Drug Conc. (Cut-off range)	MET1000	
	POS/+	NEG/-
0% Cut-off	0	30
-50% Cut-off	0	30
-25% Cut-off	6	24
Cut-off	12	18
+25% Cut-off	29	1
+50% Cut-off	30	0
Drug Conc. (Cut-off range)	THC50	
	POS/+	NEG/-
0% Cut-off	0	30
-50% Cut-off	0	30
-25% Cut-off	0	30
Cut-off	9	21
+25% Cut-off	13	17
+50% Cut-off	30	0

Analytical Specificity

The following table lists the concentration of compounds (ng/mL) that are detected positive in urine by FrenoVO One Step MET-THC Urine Rapid Test at 5 minutes.

Compounds for M line	Conc. ng/ml
d-Methamphetamine	1,000
p-Hydroxymethamphetamine	30,000
Mephentermine	50,000
l-Methamphetamine	8,000
d,l-3,4-Methylenedioxymethamphetamine (MDMA)	2,000
Compounds for T line	Conc. ng/ml
11-nor- Δ^9 -THC-9 COOH	50
Cannabinol	20,000

11-nor- Δ^8 -THC-9 COOH	30
Δ^8 -THC	15,000
Δ^9 -THC	15,000














Cross-Reactivity

A study was conducted to determine the cross-reactivity of the test with compounds in either drug-free urine or Methylenedioxyamphetamine positive urine. The following compounds show no cross-reactivity when tested with FRENOVO One Step MET-THC Urine Rapid Test at a concentration of 100 µg/mL.

Non Cross-Reacting Compounds		
4-Acetamidophenol	Ethyl alcohol	Orphenadrine
Acetone	Ethyl-p-aminobenzoate	Oxalic acid
Acetophenetidin	Etodolac	Oxolinic acid
Acetylsalicylic acid	Famprofazone	Oxymetazoline
Albumin	Fenoprofen	Papaverine
alpha-Naphthaleneacetic Acid	Fluoxetine	Pemoline
Aminopyrine	Furosemide	Penicillin
Amoxapine	Gentisic acid	Pentazocine
Amoxicillin	d-Glucose	Phenelzine
Ampicillin	Guaiacol Glyceryl Ether	Pheniramine
ApoMethylenedioxyamphetamine	Hemoglobin	Phenothiazine
Ascorbic acid	Hydralazine	Prednisolone
Aspartame	Hydrochlorothiazide	Prednisone
Atropine	Hydrocortisone	d,l-Propanolol
Benzilic acid	o-Hydroxyhippuric acid	Quinacrine
Benzoic acid	3-Hydroxytyramine	Quinidine
Benzylamine	Ibuprofen	Quinine
Brompheniramine	lproniazid	R(-) Deprenyl
Caffeine	Isoproterenol	Riboflavin
Cannabidiol	Isoxsuprine	Salicylic acid
Chloral Hydrate	Kanamycin	Serotonin
Chloramphenicol	Ketoprofen	Seroquel
Chloroquine	Labetalol	Sertraline
Chlorothiazide	Lidocaine	Sodium Chloride
Chlorpromazine	Lindane	Sulfamethazine
Chlorprothixene	Lithium	Sulindac
Cholesterol	Loperamide	Tetracycline
Cimetidine	l-Thyroxine	Tetrahydrocortison-3-acetate
Clonidine	Meperidine	Tetrahydrozoline
Cortisone	Meprobamate	Theophylline
Creatinine	Methaqualone	Thiamine
Deoxycorticosterone	Methoxyphenamine	Thioridazine
Dextromethorphan	Methylphenidate	Tolbutamide
Diclofenac	Metoprolol	Trans-2-phenylcyclopropylamine
Dicyclomine	N-Acetylprocainamide	Trazodone
Diflunisal	Nalidixic acid	Triamterene

Digoxin	Nalorphine	Trifluoperazine
4-Dimethylaminoantipyrine	Naproxen	Trimethoprim
Diphenhydramine	Niacinamide	d,l-Tryptophan
5,5-Diphenylhydantoin	Nifedipine	d,l-Tyrosine
EMDP	Nimesulide	Uric acid
Erythromycin	Norethindrone	Verapamil
β-Estradiol	Noscapine	Zomepirac
Estrone-3-sulfate	d,l-Octopamine	-----

INDEX OF SYMBOLS

	In vitro diagnostic medical device		single-use, Please don't reuse it
	Use-by date		Consult instructions for use
	Cautions		Manufacturer
	Temperature limit		Batch code
	Date of manufacture		Keep Dry
	Avoid overexposure to the sun		Don't use the product when the package is damaged
	Biological risks		



Hangzhou Frenovo Biotech Co., Ltd.

Address: Room 401, Building 26, Room 401&301, Building 27, No.488-1, Donghu North Road, Donghu Street, LinPing District, Hangzhou City, Zhejiang Province, China.

Tel: +86-571-89170657

Email: business@frenovo.com

INSTRUCTION APPROVAL AND REVISION DATE

Revision Date: 2025.10.22

Approval Date: 2025.10.22

Date of Issue: 2025.10.22